

Käfer

CERTIFICAT D'ETALONNAGE No 841193

KALIBRIERSCHEIN

CALIBRATION CERTIFICATE

Messuhr Comparateur Dial Indicator

No de série
Seriennummer
Serial Number

841193

Course de mesure
Meßspanne
Measuring Range

12.5 mm

Résolution
Auflösung
Resolution

0.001mm

Force de mesure
Messkraft
Measuring Force

0.65 - 0.90 N

Précourse
Anhub
Pretravel

0.201mm


Etalonné avec
Kalibriert
Calibrated with

Unit No 026 / Probe No 1901

Nous certifions que cet instrument a été fabriqué et contrôlé selon ses normes internes de Qualité.
Les étalons utilisés ont une traçabilité reconnue par METAS (Office Fédéral de METrologie et Accréditation Suisse).

Wir bestätigen, dass dieses Instrument gemäss seinen internen Qualitätsnormen hergestellt und geprüft wurde.
Die verwendeten Referenzmasse verfügen über eine anerkannte Rückverfolgbarkeit durch METAS (Eidgenössische Amt METrologie und Akkreditierung Schweiz).

We certify that this instrument has been manufactured according to our Standard of Quality and tested in reference with master of certified traceability by METAS (federal office of METrology and Accreditation Switzerland).

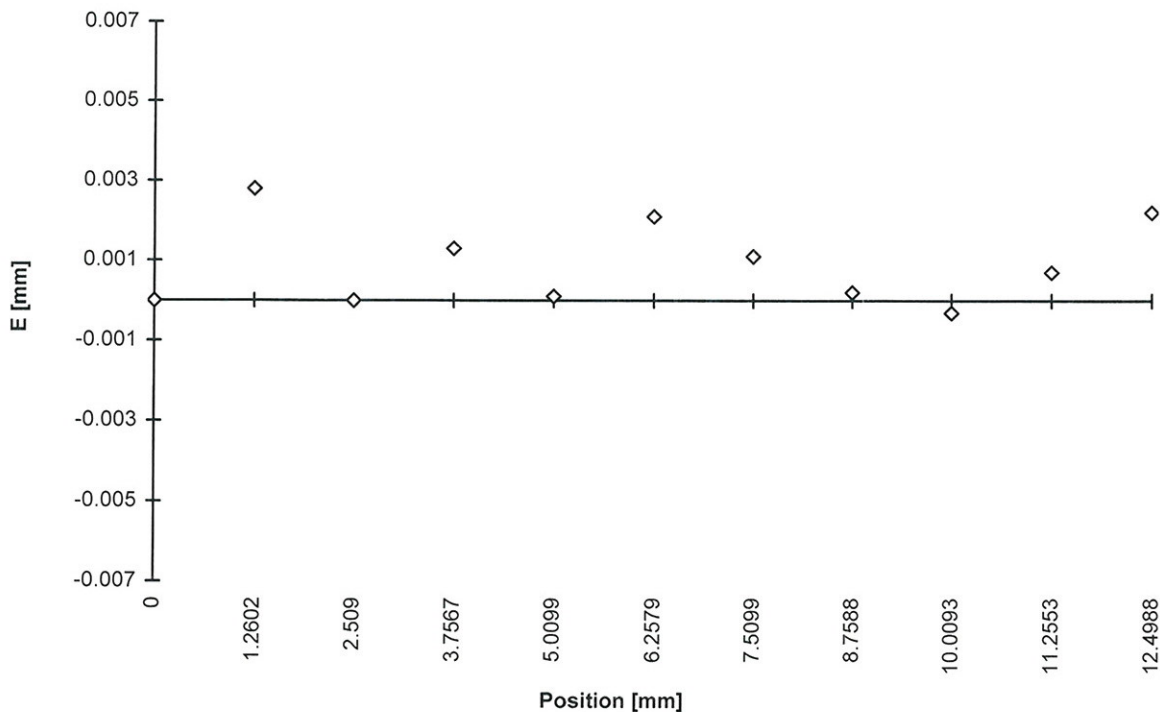

Erreur Maximum
Maximale Abweichung
Maximum Error

3µm

Incertitude de mesure (U95%)
Uncertainty of measurement (U95%) $\pm 0.77\mu\text{m}$
Messunsicherheit (U95%)

Contrôleur / Prüfer / Inspector

D. Schaller 3-oct-08